


Preliminary transmission measurement of borofloat window


Sean Stoll

BNL

4/9/2025

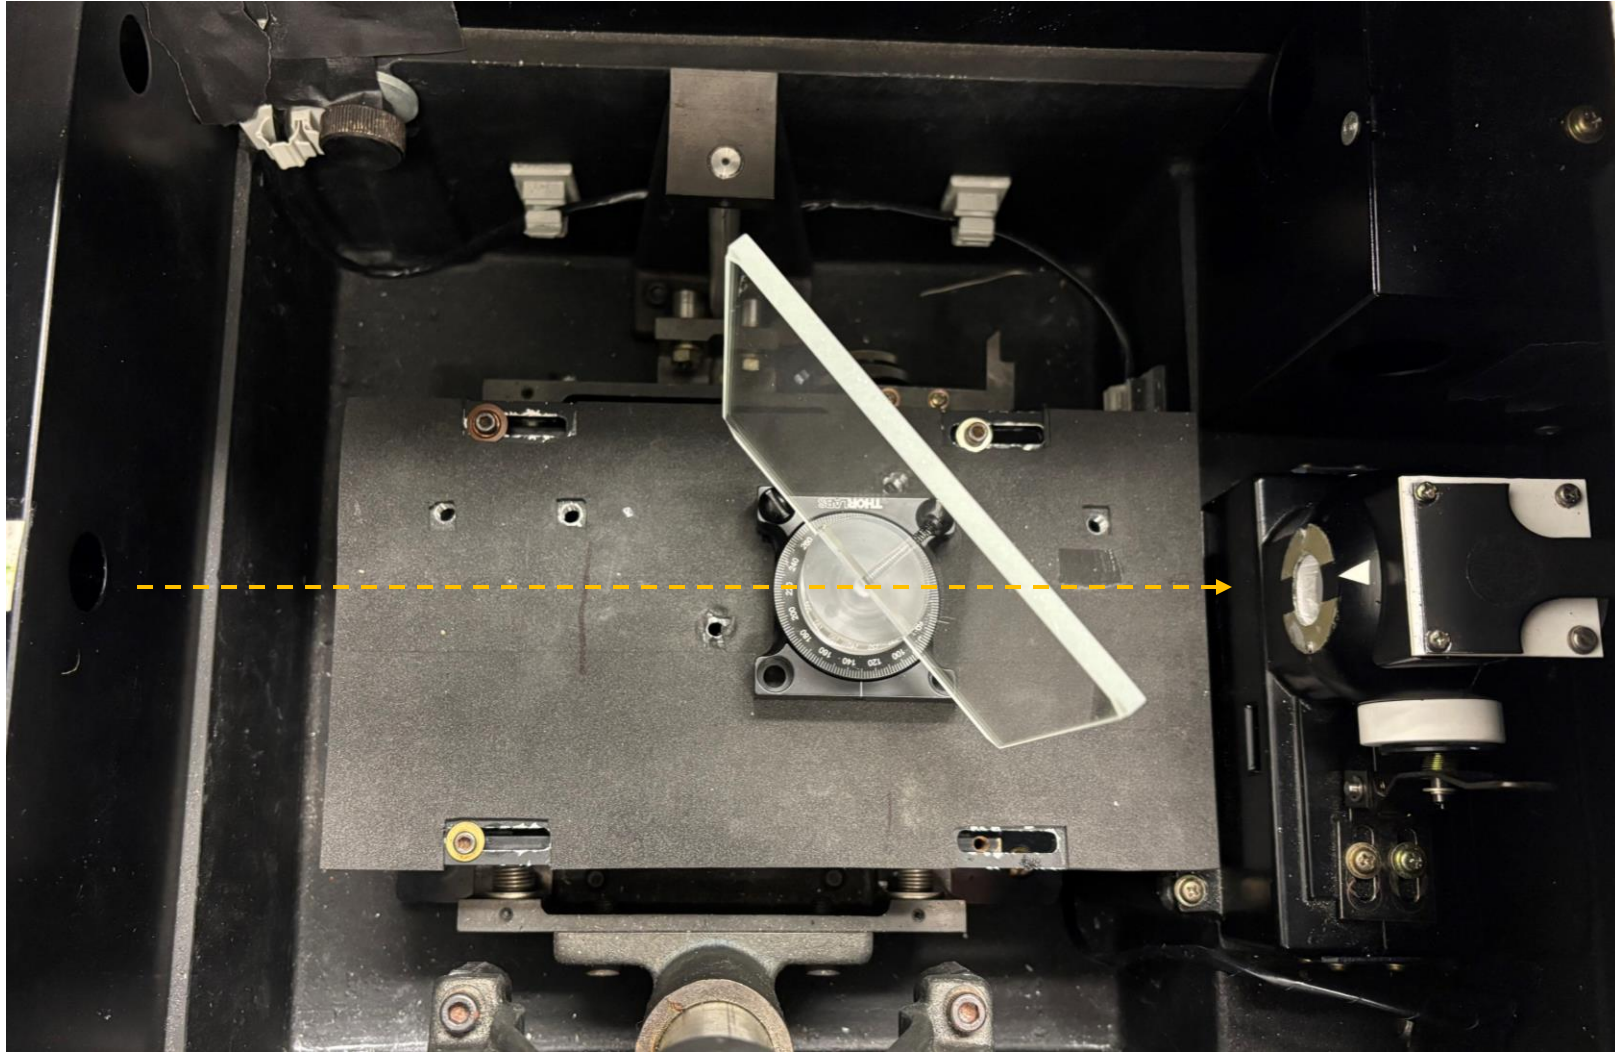

Window mounted in Hitachi spectrophotometer chamber

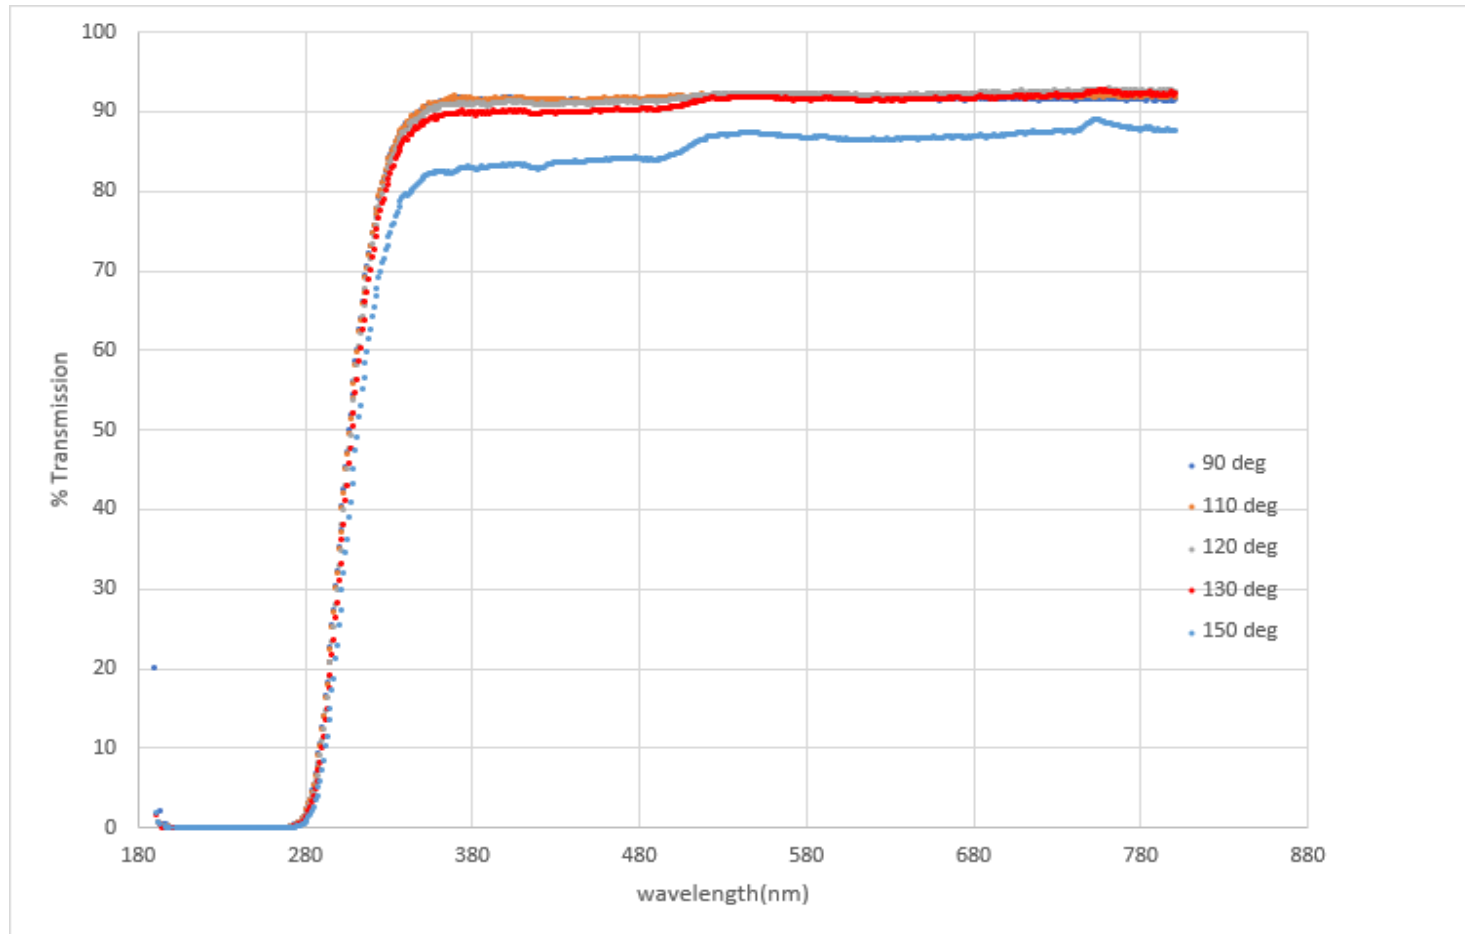

Preliminary measurement of %transmission vs wl for various angles of incidence.

Will revisit measurement today.