




HRPPD test stand in 2-233

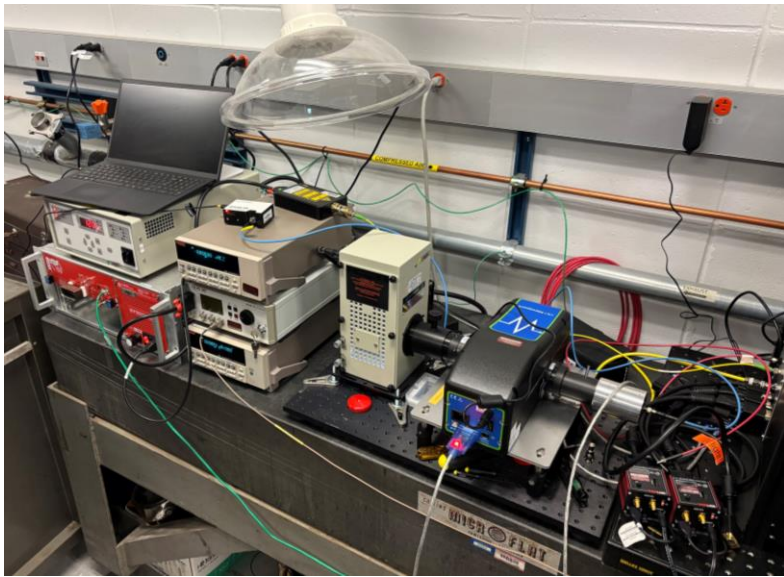


Full equipment setup on test bench.

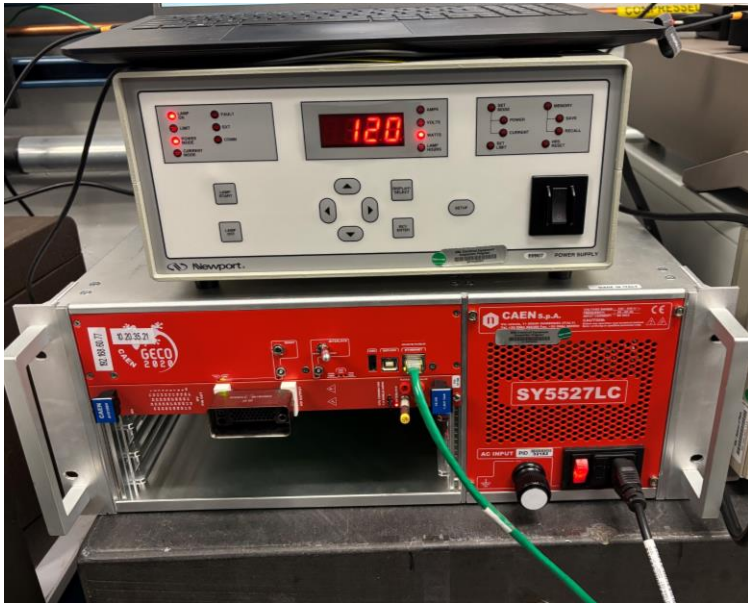


Light source power supply and
Caen crate for HRPPD power module

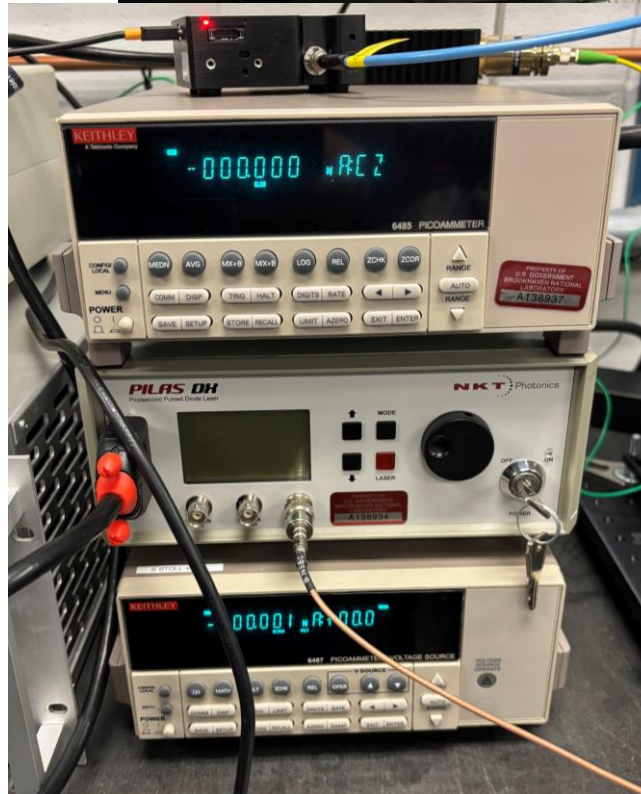


Kiethley 6487 voltage source / picoammeters
PiLas Laser Controller

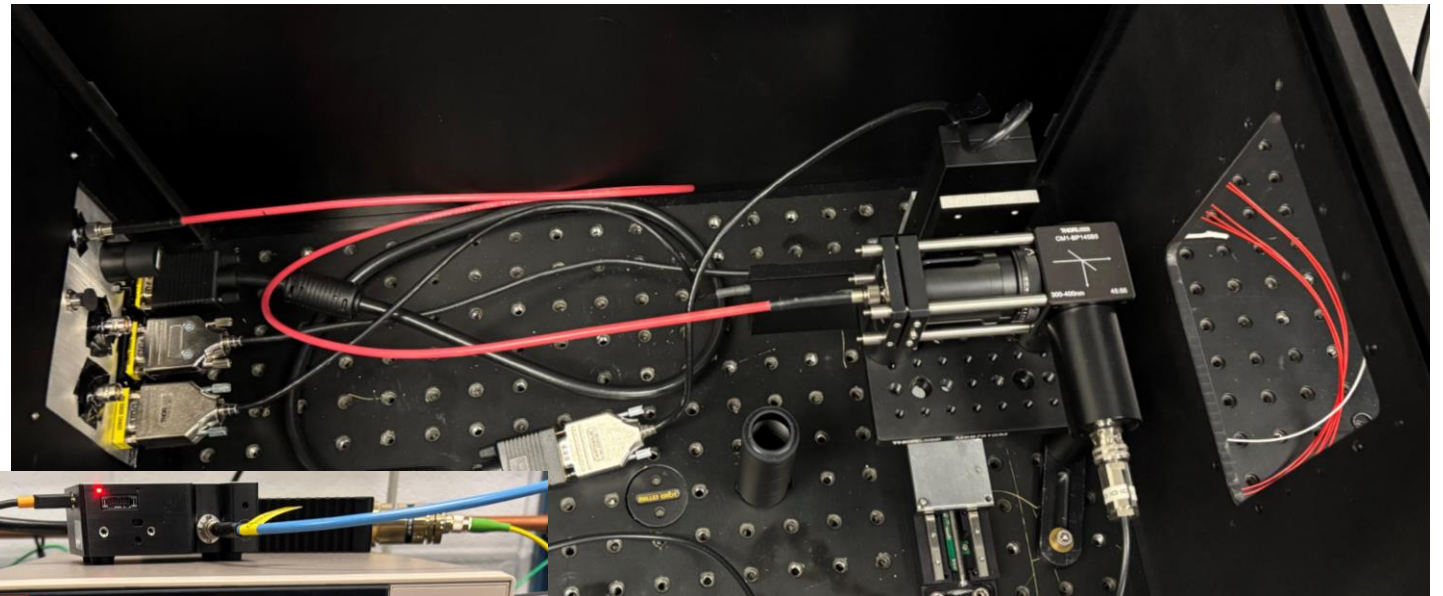

Inside darkbox - scanner head with light input fiber
And monitoring photodiode

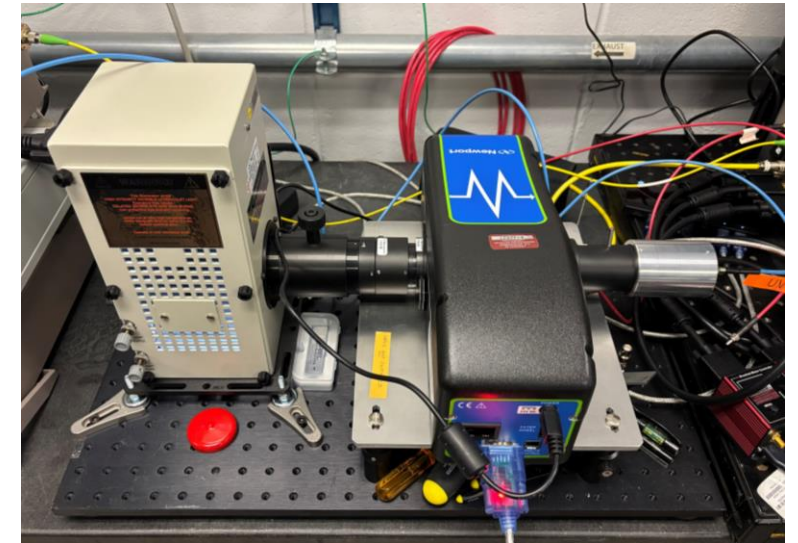

Newport/Oriel Light source and monochromator

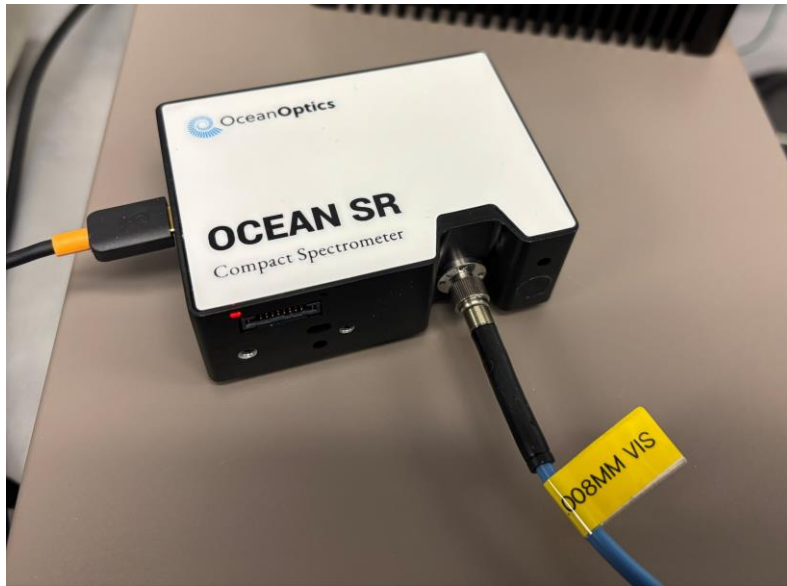

Ocean Optics Fiber Spectrometer

Oceanview Spectrometer

Utility Software

Monochromator set to 500.0nm

Measured peak is ~501nm

